


1 *Optical crystal on the PCI test bench for measuring the residual absorption.*

2 *Schematic setup of a photothermal common-path interferometer. A weak probe beam detects the effects of an intense pump beam passing through a sample.*

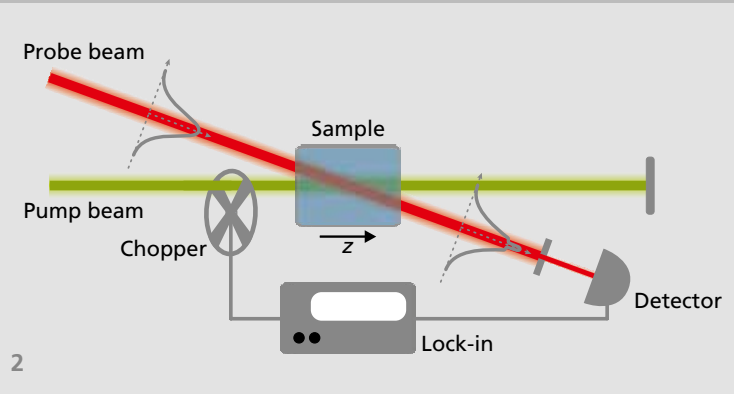

ABSORPTION SPECTROSCOPY OF TRANSPARENT OPTICAL MATERIALS

High powers need high purities: The current development of high-power lasers calls for better quality assessment of optical materials for high-power applications. In bulk materials for lenses and mirrors, in dielectric coatings or nonlinear-optical components, material imperfections or impurities may lead to residual absorption. Under high laser intensities, absorption coefficients of 1000 ppm/cm or below may cause local heating, resulting in component malfunction or even damage.

Several techniques have been developed to detect residual absorption in highly transparent optical materials down to 10 ppm/cm or even less. At such high sensitivity levels, indirect techniques are the only option: They either detect the resulting temperature increase or secondary effects caused by the intense laser illumination, i.e. thermal expansion or refractive index changes.

Photothermal common-path interferometry (PCI)

Photothermal common-path interferometry (PCI) is a highly sensitive method, based on a pump-probe-technique: A strong continuous-wave (cw) pump beam is focused into the sample, heating it locally due to light absorption. The resulting local change of the refractive index causes refraction and diffraction effects on the crossing probe beam. This distortion is proportional to the absorption of the sample and can be measured by a lock-in technique.

Translating the sample in z-direction through the interaction zone of the laser beams delivers spatially resolved PCI data that provide values for both bulk and surface absorption.


Fraunhofer Institute for Physical Measurement Techniques IPM

Georges-Köhler-Allee 301
79110 Freiburg, Germany


Contact

Dr Frank Kühnemann
Nonlinear Optics and Quantum Sensing
Phone +49 761 8857-457
frank.kuehnemann@ipm.fraunhofer.de

www.ipm.fraunhofer.de/en

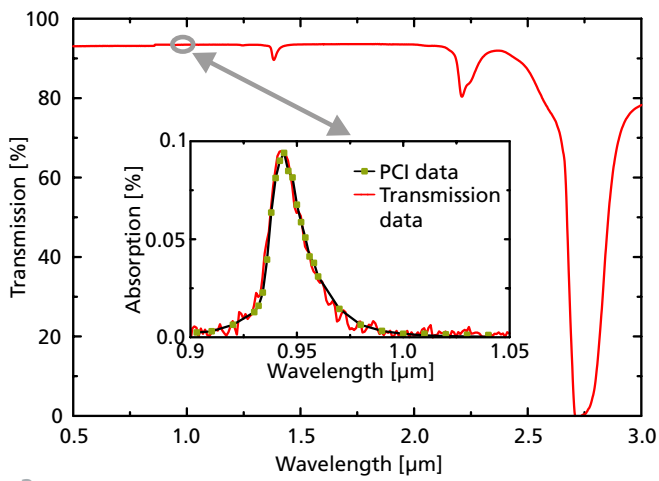

3

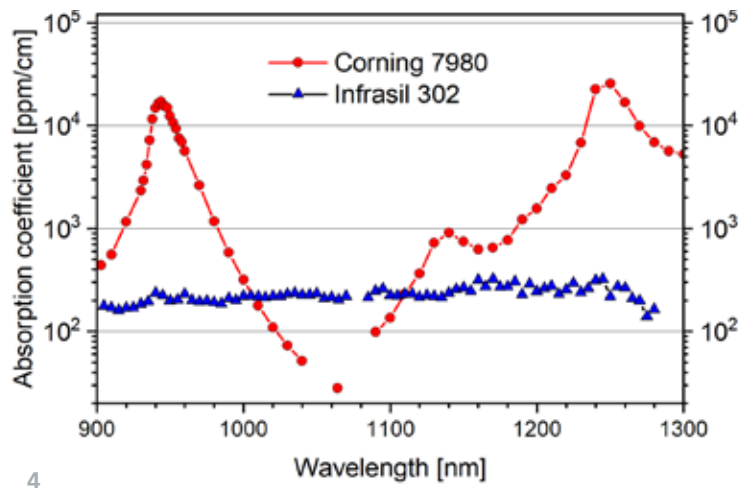

4

3 Absorption calibration of a fused silica sample using the weak OH absorption peak at 940 nm. Inset: PCI-data vs. absorption data from transmission.

4 Absorption spectra of two fused silica types. Corning 7980: pronounced OH absorption bands; Infrasil 302: broad background absorption due to metal impurities.

5 Wavelength ranges available for PCI measurements.

6 PCI scan of a fused-silica sample with AR coatings on both surfaces. The sample is moved through the interaction zone of the two laser beams. The PCI signals are then converted into absorption values for bulk and surface using material-specific conversion coefficients.

Our advantage

Traditionally, high-sensitivity absorption measurements are performed at the fixed wavelengths of high-power lasers, since these are the most relevant ones for the use of such optical components. Fraunhofer IPM goes one step further by combining PCI with in-house developed cw optical parametric oscillators (OPO) as pump lasers. This way, absorption spectra of materials and components can be provided that cover large wavelength ranges.



Calibration

PCI measurements yield only relative absorption data, as it is the case with all high-sensitivity techniques. Hence, calibration is required for absolute measurements. Utilizing the tunability of the OPOs by Fraunhofer IPM, the absorption

features present in the sample, e.g. OH absorption in fused silica, may be recorded with the PCI spectrometer. Comparing these measurements with transmission data provides the required calibration information. This approach avoids the need for doped samples. It results in a higher accuracy of the absorption calibration and facilitates the analysis of new materials.

Cross-system validation

In addition to PCI, Fraunhofer IPM has access to two other methods for the sensitive detection of residual absorptions in highly transparent materials. Comparing, e.g., PCI results for a sample of lithium niobate (LiNbO_3) with data from photoacoustic absorption measurements and total loss data from a LiNbO_3 whispering gallery resonator shows good agreement over more than four orders of magnitude.

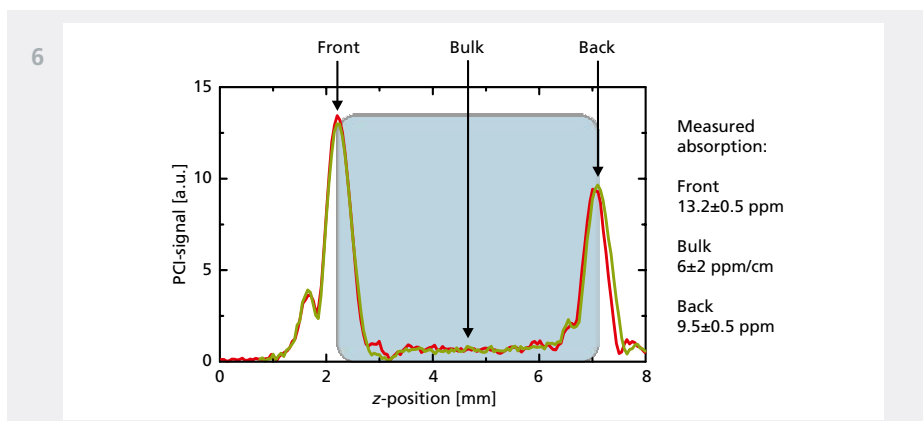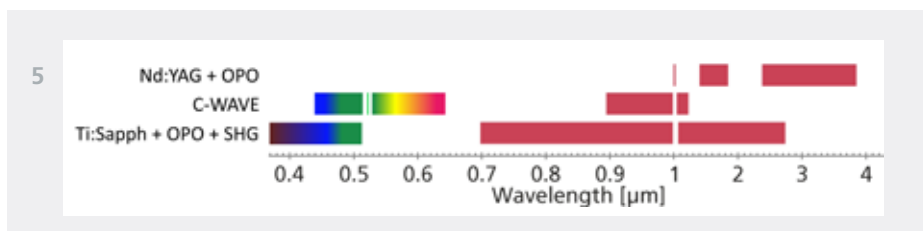

SPECIFICATIONS

- **Detection limits**
 10^{-5} - 10^{-6} cm^{-1} for bulk absorption
 10^{-6} - 10^{-7} cm^{-1} for coatings
(wavelength and material dependent)
- **Spatial resolution**
50 μm transversal
700 μm lateral
- **Measurement of AR and HR coatings, lenses and mirror blanks**

OUR PORTFOLIO

- Service measurements
- Quality control for supply-chain support
- Delivery of customized measurement systems